New vision of imaging



Phantom

for ultrasound

Instructions and User Guide




This guide will help you to understand how to handle and to increase the durability of you Phantom. Next, we present some important information about the Anesthesia Phantom:

- Always keep our Phantom in the storage case and at room temperature. Note.: Exposure to temperatures above 30°C (86°F) for long periods can provoke deformations and loss of properties;
- 2. When training, remove only the packaging lid, keeping the Phantom in the original base;
- 3. After training, clean your Anesthesia Phantom with paper towel removing excess gel. Following, wash it in running water without removing it from the base. Obs.: Never store your Phantom with excess gel. This can cause bad smell reducing product durability;
- 4. Never use soaps or sponges for cleaning your phantom. They can damage your product!
- 5. After cleaning, store your Phantom according to instructions in item I;
- 6. VI. The Anesthesia Phantom is a product for didactic purposes, made ONLY for medical trainings. If you have any doubts contact us through our relationship channels.

## Anesthesia phantom

## About your Anesthesia phantom

- 1. We recommend the utilization of new and sharp needles not larger than 21G. During training, repositioning of needles can cause needle tracks. To reduce this marks its advisable an interval of 24 hours until the next use;
- 2. When using the needles described above, Phantoms allow movements up to 30 degrees relative to product surface. Avoid long needle movements, they can diminish your product's durability;
- 3. III. We do not recommend injecting or removing any types of materials during utilization. If you have this need, get in contact with us;
- 4. IV. The Anesthesia Phantom are equipped with six structures that simulate three nerves and three veins alternately arranged within the model. Such structures, enable the training of procedures of regional anesthesia and ultrasound-guided central venous access. Below follow four ultrasound mode B images of the Anesthesia Phantom:

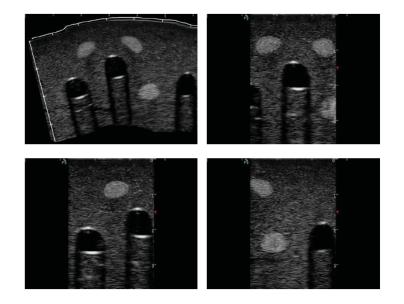

Réf.	Approximate weight	Length	Height	Width
PBD050502	700 g	17 cm	4 cm	13 cm



EDM Imaging 1 rue des Boisseliers 95330 Domont - France Tél. (+33) 01 30 11 83 00

www.edm-imaging.com